V-CHEK

CE 2854

SUITABLE FOR SELF-TESTING USE

2019-nCoV Ag Rapid Test Kit

(Immunochromatography)



1 Test/Kit



5 Tests/Kit




25 Tests/Kit


High accuracy

Easy to use


Nasal self-test

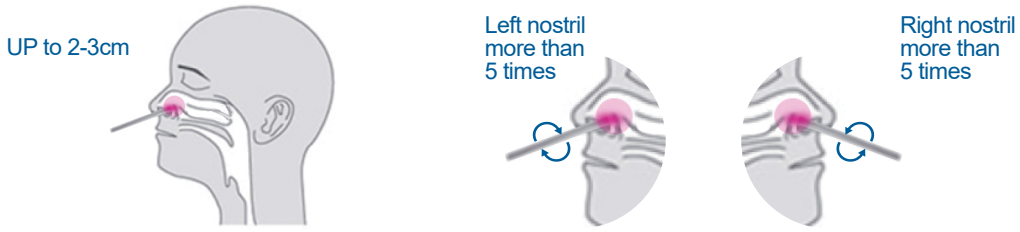

1 Gentle sampling only 2-3 cm from the anterior nasal cavity.

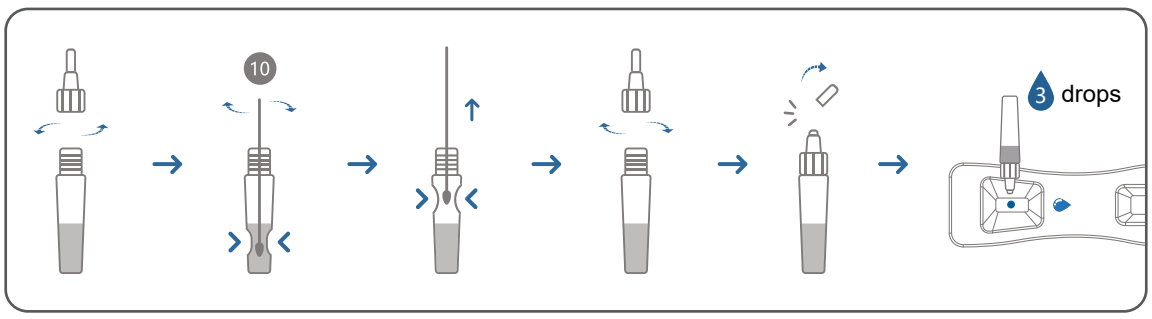

2 Dip the tip of the swab with the sample into the buffer tube and rotate 10 times. Drop 3 drops of buffer into the sample well.

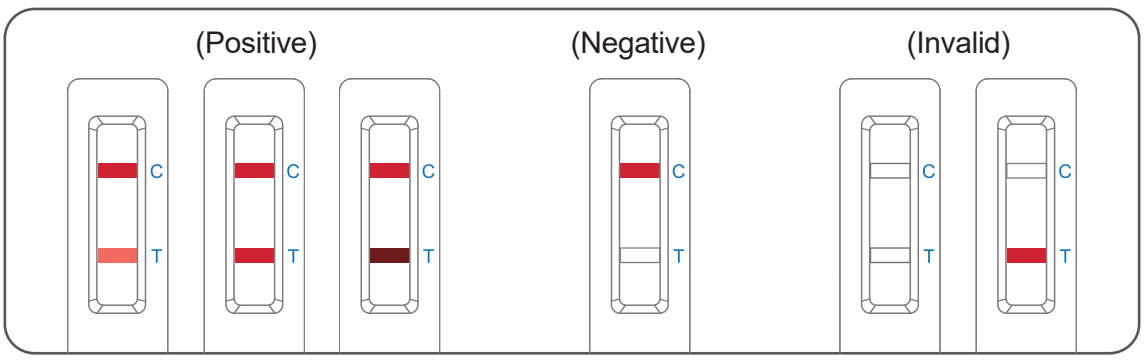

3 Read the result at 15 minutes. Do not read the result after 20 minutes.

PERFORMANCE CHARACTERISTIC

2019-nCoV Ag Rapid Test Kit (Immunochromatography)	Comparative RT-PCR Test Result		
	Positive (+)	Negative (-)	Total
Detected Positive	280	3	283
Detected Negative	10	515	525
Gesamt	290	518	808
Sensitivity: 96.55%, 95% CI (93.77, 98.12)			
Specificity: 99.42%, 95% CI (98.31, 99.80)			
Accuracy: 98.39%, 95% CI (97.27, 99.06)			

DoChek 德成生物

Guangzhou Decheng Biotechnology Co., LTD
Room 218, Building 2, No.68, Nanxiang Road, Science City, Huangpu District, 510000, Guangzhou P.R.China
TEL:+86-020-82557192 Email:service@dochekbio.com www.dochekbio.com